

Makrite(麦特瑞)N95—9500



N95 NIOSH RESPIRATORS

9500
Comfort Series

The 9500 Comfort Series of NIOSH approved respirators is the "standard" for all the industries in which these products are used. This is the basic N95 product developed to compete with similar appearing disposable respirators. By far, this cone style of N95 mask is the most widely used mask in all work environments. These models have been designed to easily meet NIOSH's stringent approval requirements for breathing resistance and filtration efficiency. Most companies interested in adding N95 respirators to their line of business will select either our 9500 Comfort Series or the alternative MK Comfort Series, or the new 9600 Series as the focal point around which to build a disposable respirator line.



ITEM	DESCRIPTION	PACKAGING	APPROVAL
*9500-N95	N95 Cone Respirator	20 masks/box; 12 boxes/case	TC-84A-5411
*9500-N95S	N95 Cone Respirator	20 masks/box; 12 boxes/case	TC-84A-5463
9500V-N95	N95 Cone Respirator with Exhalation Valve	10 masks/box; 12 boxes/case	TC-84A-5460
9500-N95OV	N95 Cone Respirator (Nuisance Organic Vapors)	10 masks/box; 12 boxes/case	TC-84A-5525
9500-N95OV	N95 Cone Respirator with Exhalation Valve (Nuisance Organic Vapors)	10 masks/box; 12 boxes/case	TC-84A-6954
8810S	N95 Cone Respirator	20 masks/box; 12 boxes/case	TC-84A-6953

* Cleared by the Food and Drug Administration for use as a Surgical N95 Respirator. FDA 510(k): K020474

Makrite(麦特瑞)品牌介绍



***"Makrite Industries – perhaps, the premier manufacturer
of disposable face masks in the Far East"***

As a face mask manufacturer and distributor for over 30 years, Makrite strives to provide the best possible respiratory protection products to our valued customers worldwide. We set up manufacturing in China to produce specially designed disposable face masks and particulate respirator masks to meet governmental requirements in many countries.

To produce our N95 masks and CE marked masks, we work closely with NIOSH (National Institute for Occupational Safety and Health) and the FDA (Food and Drug Administration) in the U.S., and with INSPEC in England to insure our products are up-to-date and meet all necessary U.S. and CE requirements. We also have product approvals in Japan, Australia and New Zealand.

We are proud to be one of the world's premier manufacturers of disposable face masks. Founded in 1980 in Taipei, Taiwan, we have always strived to provide the best possible face mask products to our valued customers worldwide. Our products are now used in the medical, industrial, automotive and consumer markets all over the world – keeping workers safe and productive, while also keeping costs down for the purchaser.

NIOSH (the National Institute for Occupational Safety Hazards) in the U.S. is a frequent visitor to our manufacturing facility. We face frequent audits, and have outstanding results to show for them. We now produce over 40 NIOSH



approved safety products, many of which are produced on high speed automatic specially designed machinery to insure consistency from one mask to the next. Our approvals from NIOSH indicate our adherence to the strict quality and production controls.

Similarly, we have many European and other nation government approvals again reflecting the quality of our products and the stringent control of our manufacturing plant.

Many well known companies have chosen us to be their supplier of these masks for their own private brand packaging, based on our customer service, product quality and competitive prices.

With our headquarters in Taiwan, we now have significant satellite offices in Korea, Japan, U.S and Singapore. We attend or exhibit at all the major face mask related trade shows worldwide. We welcome the opportunity to work with our customers to develop exclusive, custom-designed face mask products as well as special distribution partnerships. Marketing and technical support are available through any of our offices.

Finally, and most important, we would like to thank our customers, suppliers and employees for all their support during the last 30+ years.

Sincerely your,
The Makrite Family

Mission Statement: To make a positive difference in the businesses of our customers through the best possible customer service, quality of products, and competitive prices.





营业执照

(副本) (1-1)

统一社会信用代码 91421200MA491WCQ4U

名称 知腾工业（湖北）有限公司
类型 有限责任公司(外国法人独资)
住所 湖北赤壁高新区光谷产业园纵二路1号
法定代表人 卓庚霖
注册资本 柒佰伍拾万美元整
成立日期 2017年11月08日
营业期限 2017年11月08日至2047年11月07日
经营范围 生产、销售各类无纺布口罩；自动设备设计、制造及整厂输出规划服务；生产、销售各类硅胶面罩、相关副件及注塑零配件、劳保用品（口罩、防护服、安全眼镜）；生产销售各类化纤布、洗涤布桌巾及相关桌上用品；化纤布浴帘、塑胶桌布、床套、户外套、塑料卷料桌巾、空滤产品的制造、销售。（涉及许可经营项目，应取得相关部门许可后方可经营）



企业应当每年1月1日至6月30日，
报送年度报告，并向社会公示。

登记机关

2017年11月08日



LA证书

特种劳动防护用品安全标志

证

书

特种劳动防护用品安全标志管理中心



特种劳动防护用品安全标志证书

知腾工业（湖北）有限公司

生产的特种劳动防护用品，经审查，符合特种劳动防护用品安全标志规定的要求，特发此证。

具体产品名称、产品类别、企业产品规格型号及标识编号见特种劳动防护用品安全标志证书附件。

证书编号：LA-2019-2010



有效期至 2024年12月30日

年 检 情 况

2020年	2021年	2022年	2023年
-------	-------	-------	-------



二〇一九年十二月三十一日



Certificate of LA Mark of
Personal Protective Equipment

This is to certify that the Personal Protective Equipments(detail of the products name,catagory,specification,model and mark numbers see appendix of LA Mark Certificate) manufactured by **MAKRITE HUBEI INDUSTRIAL CO.,LTD** meet the requirements of LA Mark.

Certificate number: **LA-2019-2010**

Date of issue: **Dec.31,2019**


Date of expiry: **Dec.31,2024**

**LA MARK CENTER OF
PERSONAL PROTECTIVE EQUIPMENT**

产品名称	产品类别	企业产品规格型号	标识编号
1. 自吸过滤式防颗粒 物呼吸器	随弃式面罩 有呼气阀	9500V-KN90	19-42-201016
	KN90		
	随弃式面罩 有呼气阀	9500V-KN95	
	KN95		
	随弃式面罩 有呼气阀	800-KN100	
	KN100		
	随弃式面罩 有呼气阀	MK710V-KP95	
	KP95		
	随弃式面罩 无呼气阀	9500-KN90	
	KN90		
以下空白	随弃式面罩 无呼气阀	9500-KN95	
	KN95		
	随弃式面罩 无呼气阀	810-KN100	
	KN100		
	随弃式面罩 无呼气阀	MK710-KP95	
	KP95		



Makrite(麦特瑞)包装




箱规: 67*30*42cm

重量: 6kg

1箱400支 (20小盒)



包装图



1. 纸盒小大 : 200X140X130mm
2. 包装方式 : 20PCS/盒, 20盒/箱
3. 纸箱大小 : 67X30X42cm
4. 重量 : 6公斤/箱



NIOSH检测报告

DEPARTMENT OF HEALTH & HUMAN SERVICES

Public Health Service

NIOSH Reference: TN-17685
Mfr. Reference: MAK-1105

Centers for Disease Control
and Prevention (CDC)
National Institute for Occupational
Safety and Health (NIOSH)
National Personal Protective
Technology Laboratory (NPPTL)
P.O. Box 18070
Pittsburgh, PA 15236-0070
Phone: 412-386-4000
Fax: 412-386-4051

April 19, 2011

Mr. Alexander Freedman, President
Makrite Industries Inc.
236 Upland Avenue
Newton Highlands, Massachusetts 02461-2003

Dear Mr. Freedman:

The National Institute for Occupational Safety and Health (NIOSH) has reviewed your request accepted March 8, 2011. This request was for an approval of the model 9500-N95 filtering facepiece air purifying respirator for protections against particulates at a N95 filter efficiency level, reference the assembly matrix MAK1105AM1.xls.

This request is granted. Approvals are granted only for documentation written in the English language. It is the manufacturer's responsibility to correctly translate materials desired in languages other than English. The approval number TC-84A-5411 has been assigned. This respirator is approved for protections against particulates at a N95 filter efficiency level (N95).

The CD enclosed with this letter contains the final respirator label. The abbreviated label has been accepted as submitted. The cautions and limitations which apply to this approval are on the approval label. Only those assemblies affected by this request, or where new approval numbers are assigned, apply to this approval action. Production approval labels cannot include information on unapproved configurations.


The approved assembly consists of the parts as listed on the approval label and the assembly matrix. Parts are to be marked with the numbers indicated on the approval label in a legible and permanent manner (marking cannot be removed without evidence of its previous presence).

This certificate of approval is not an endorsement of the respirator by NIOSH, and such endorsement shall not be stated or implied in advertisements or other publicity. However, you may publicize the fact that the respirator has met the requirements of Title 42, *Code of Federal Regulations*, Part 84 (42 CFR 84).

Page 2 – Mr. Alexander Freedman – TN-17685

No changes may be made to any respirators and accompanying documentation without prior written approval of NIOSH. Requests for changes must be submitted to NIOSH and a modification of this approval must be granted before changes are made.

Sincerely yours,

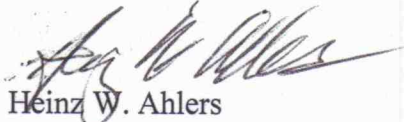A handwritten signature in dark ink, appearing to read "Heinz W. Ahlers", is written over the typed name.

Heinz W. Ahlers
Chief, Technology Evaluation Branch
National Personal Protective Technology Laboratory

Enclosures



National Institute for Occupational Safety and Health
National Personal Protective Technology Laboratory
Technology Evaluation Branch
Certification, Evaluation and Testing Section
P.O. Box 18070
Pittsburgh, PA 15236

TEST REPORT

Task Number: TN-17685

Manufacturer: Makrite Industries, Inc.

Prepared by: Jeremy Brannen

Tests Conducted by: Jeremy Brannen

Date: March 30, 2011

Respirator Tested: 9500-N95

Background Information

In an application accepted March 8, 2011 Makrite Industries requested an approval of the model 9500-N95 filtering facepiece air purifying respirator for protections against particulates at a N95 filter efficiency level, reference the assembly matrix MAK1105AM1.xls.

Tests Assigned

<u>Test Description</u>	<u>STP Number</u>	<u>Reference</u>
A. Exhalation Resistance Test	RCT-APR-STP-0003	84.180
B. Inhalation Resistance Test	TEB-APR-STP-0007	84.180
C. Sodium Chloride (NaCl) N95 Test	TEB-APR-STP-0059	84.181

Overall Results

The items tested passed laboratory testing.

Individual Test Results

See attached test data sheets.

**National Institute for Occupational Safety and Health
Respirator Branch
Test Data Sheet**



Task Number: TN-17685

Reference No.: CFR 84.180

Test: Exhalation Resistance Test

STP No.: 3

Manufacturer: Makrite Industries, Inc.

Filter Type: Filter Only

Item Tested: 9500-N95

Sample	呼气标准 Maximum Allowable Resistance (MM of H2O)	实际数据 Actual Resistance (MM of H2O)	Result
	Exhalation	Exhalation	
1	25	5.6	PASS
2	25	5.3	PASS
3	25	5.6	PASS

Overall Result: PASS

Comments:

Was all equipment verified to be in calibration throughout all testing?

☒ Yes ☐ No

Signature:

Engineering Technician

Date: 3/30/2011

National Institute for Occupational Safety and Health
Respirator Branch
Test Data Sheet



Task Number: TN-17685

Reference No.: CFR 84.180

Test: Inhalation Resistance Test

STP No.: 7

Manufacturer: Makrite Industries, Inc.

Item Tested: 9500-N95

Filter Type: Filter Only

Sample	标准阻力数据	实际阻力数据	Result
	Maximum Allowable Resistance	Actual Resistance	
	(MM of H2O)	(MM of H2O)	
Inhalation	Inhalation		
1	35	6.9	PASS
2	35	6.9	PASS
3	35	6.9	PASS
Overall Result: PASS			

Signature:

Engineering Technician

Date: 3/30/2011

Task Number: TN-17685

Reference No.: CFR 84.180

Test: Inhalation Resistance Test

STP No.: 7

Manufacturer: Makrite Industries, Inc.

Item Tested: 9500-N95

Comments:

Was all equipment verified to be in calibration throughout all testing?

☒ Yes ☐ No

Signature:



Engineering Technician

Date: 3/30/2011

National Institute for Occupational Safety and Health
Respirator Branch
Test Data Sheet



Task Number: TN-17685

Reference No.: CFR 84.181

Test: Sodium Chloride (NaCl) - N95

STP No.: 59

Manufacturer: Makrite Industries, Inc.

Item Tested: 9500-N95

初始阻力

标准泄漏率

初始泄漏率

最高泄漏率

Filter	Flow Rate	Initial Filter Resistance	Maximum Allowable Percent Leakage	Initial Percent Leakage	Maximum Percent Leakage	结果 Result
1	85	7.8	5.00	0.373	0.426	PASS
2	85	7.9	5.00	0.375	0.426	PASS
3	85	7.4	5.00	0.777	0.976	PASS
4	85	8.0	5.00	0.568	0.784	PASS
5	85	8.2	5.00	0.605	0.831	PASS
6	85	7.7	5.00	0.684	0.885	PASS
7	85	7.4	5.00	0.724	0.957	PASS
8	85	8.4	5.00	0.346	0.569	PASS
9	85	7.4	5.00	0.281	0.481	PASS
10	85	8.2	5.00	0.293	0.556	PASS
11	85	8.4	5.00	0.543	0.623	PASS
12	85	7.9	5.00	0.643	0.763	PASS
13	85	8.0	5.00	0.738	0.845	PASS
14	85	8.0	5.00	0.516	0.624	PASS
15	85	7.8	5.00	0.548	0.632	PASS
16	85	7.6	5.00	0.726	0.961	PASS
17	85	7.9	5.00	0.536	0.597	PASS
18	85	8.5	5.00	0.555	0.667	PASS
19	85	8.4	5.00	0.842	0.992	PASS
20	85	7.8	5.00	0.743	0.861	PASS

Overall Result: PASS

Signature:

Engineering Technician

Date: 3/30/2011

Task Number: TN-17685

Test: Sodium Chloride (NaCl) - N95

Manufacturer: Makrite Industries, Inc.

Item Tested: 9500-N95

Reference No.: CFR 84.181

STP No.: 59

Comments:

Was all equipment verified to be in calibration throughout all testing?



Yes



No

Signature:



Engineering Technician

Date: 3/30/2011

NIOSH证书



Makrite Industries, Inc.
11F-5, No. 79, SEC 1, Hsin Tai Wu Rd.
His-Chih, Taipei Hsein, Taiwan, R.O.C.
Telephone: (02)2698-2419



This respirator is only approved in the following configuration:

TC-	Protection ¹	Respirator	Cautions and Limitations ²
		9500-N95	
84A-5411	N95	X	ABCJMNOP

1. Protection

N95-Particulate Filter(95 % filter efficiency level)
effective against particulate aerosols free of oil;
time use restrictions may apply

2. Cautions and Limitations

- A - Not for use in atmospheres containing less than 19.5% oxygen.
- B - Not for use in atmospheres immediately dangerous to life or health.
- C - Do Not exceed maximum use concentrations established by regulatory standards
- J - Failure to properly use and maintain this product could result in injury or death.
- M - All approved respirators shall be selected, fitted, used, and maintained in accordance with MSHA, OSHA and other applicable regulations
- N - Never substitute, modify, add, or omit parts. Use only exact replacement parts in the configur
- O - Refer to users instructions, and/or maintenance manuals for information on use and maintenance of these respirators.
- P - NIOSH does not evaluate respirators for use as surgical masks.



FDA证书

JUL 23 2002

Food and Drug Administration
9200 Corporate Boulevard
Rockville MD 20850

Makrite Industries, Incorporated
C/O Mr. Joseph Zdrok
Joseph Z. Zdrok & Associates
24 Tower Street
Webster, Massachusetts 01570

Re: K020474

Trade/Device Name: Makrite Model 910-N95 Healthcare Particulate
Respirator and Surgical Mask
Regulation Number: 878.4040
Regulation Name: Surgical Apparel
Regulatory Class: II
Product Code: MSH
Dated: May 28, 2002
Received: May 31, 2002

Dear Mr. Zdrok:

We have reviewed your Section 510(k) premarket notification of intent to market the device referenced above and have determined the device is substantially equivalent (for the indications for use stated in the enclosure) to legally marketed predicate devices marketed in interstate commerce prior to May 28, 1976, the enactment date of the Medical Device Amendments, or to devices that have been reclassified in accordance with the provisions of the Federal Food, Drug, and Cosmetic Act (Act) that do not require approval of a premarket approval application (PMA). You may, therefore, market the device, subject to the general controls provisions of the Act. The general controls provisions of the Act include requirements for annual registration, listing of devices, good manufacturing practice, labeling, and prohibitions against misbranding and adulteration.

If your device is classified (see above) into either class II (Special Controls) or class III (PMA), it may be subject to such additional controls. Existing major regulations affecting your device can be found in the Code of Federal Regulations, Title 21, Parts 800 to 898. In addition, FDA may publish further announcements concerning your device in the Federal Register.


Please be advised that FDA's issuance of a substantial equivalence determination does not mean that FDA has made a determination that your device complies with other requirements of the Act or any Federal statutes and regulations administered by other Federal agencies.

You must comply with all the Act's requirements, including, but not limited to: registration and listing (21 CFR Part 807); labeling (21 CFR Part 801); good manufacturing practice requirements as set forth in the quality systems (QS) regulation (21 CFR Part 820); and if applicable, the electronic product radiation control provisions (Sections 531-542 of the Act); 21 CFR 1000-1050.

This letter will allow you to begin marketing your device as described in your Section 510(k) premarket notification. The FDA finding of substantial equivalence of your device to a legally marketed predicate device results in a classification for your device and thus, permits your device to proceed to the market.

If you desire specific advice for your device on our labeling regulation (21 CFR Part 801 and additionally 21 CFR Part 809.10 for in vitro diagnostic devices), please contact the Office of Compliance at (301) 594-4618. Additionally, for questions on the promotion and advertising of your device, please contact the Office of Compliance at (301) 594-4639. Also, please note the regulation entitled, "Misbranding by reference to premarket notification" (21CFR Part 807.97). Other general information on your responsibilities under the Act may be obtained from the Division of Small Manufacturers, International and Consumer Assistance at its toll-free number (800) 638-2041 or (301) 443-6597 or at its Internet address <http://www.fda.gov/cdrh/dsma/dsmamain.html>

Sincerely yours,

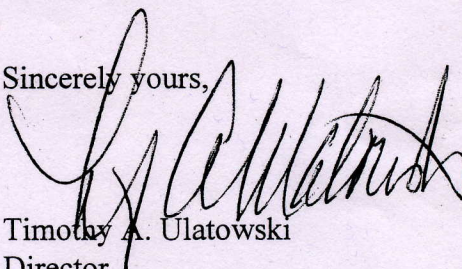

Timothy A. Ulatowski
Director

Division of Anesthesiology, General Hospital,
Infection Control and Dental Devices
Office of Device Evaluation
Center for Devices and
Radiological Health

Enclosure



质量管理体系认证证书

证书编号: 00119Q310176R2M/4400

兹证明

知勉工业股份有限公司/东莞迅安塑胶纤维制品有限公司/东莞知驛实业
有限公司

统一社会信用代码: 9144190056665074X0

台湾新北市汐止区新台五路一段七十九号十一楼之五/中国广东省东莞市塘厦镇诸佛岭工业
区/中国广东省东莞市塘厦镇诸佛岭 168 工业区广源街 12 号

建立的质量管理体系符合标准:

GB/T 19001-2016 / ISO 9001:2015

通过认证范围如下:

知勉工业股份有限公司: 劳保用品(纤维口罩、防护过滤口罩及半面罩)、家居用品(桌布、餐垫、户外套及浴帘等
相关产品)的销售。

东莞迅安塑胶纤维制品有限公司: 出口劳保用品(纤维口罩、防护过滤口罩及半面罩)的设计和生。

东莞知驛实业有限公司: 资质范围内劳保用品(纤维口罩、防护过滤口罩及半面罩)的设计和生, 家居用品(桌布、
餐垫、户外套及浴帘相关产品)的生。

首次发证日期: 2013年12月30日 本次发证日期: 2019年12月9日 有效期至: 2022年12月29日

在一个监督周期后, 本证书必须与CQC签发的监督审核合格通知书合并使用方可有效。查询证书有效状态请登陆www.cqc.com.cn。
本证书信息可在国家认证认可监督管理委员会官方网站(www.cnca.gov.cn)上查询



中国认可
国际互认
管理体系
MANAGEMENT SYSTEM
CNAS C001-M

陆梅
Signed by: Lu Mei



中国质量认证中心

中国·北京·南四环西路188号9区 100070
<http://www.cqc.com.cn>

A 0049753

2018年版



QUALITY MANAGEMENT SYSTEM CERTIFICATE

Certificate No. 00119Q310176R2M/4400

We hereby certify that

**MAKRITE INDUSTRIES INC./DONGGUAN SURE_ON PLASTIC &
FIBER PRODUCTS CO.,LTD./DONGGUAN MAKRITE
INDUSTRIES LTD.**

Unified Social Credit Code: 9144190056665074X0

11F-5, No.79, Sec 1, Xin Tai 5th Road, XiZhi Dist., New Taipei City, Taiwan,R.O.C./ ZhuFo Ling Industrial
Area,TangXia Town,DongGuan City,GuangDong,China / No.12, GuangYuan Street,168 Industrial Area, ZhuFo
Ling,TangXia Town,DongGuan City,GuanDong,China

by reason of its
Quality Management System
has been awarded this certificate for compliance with the standard

GB/T 19001-2016 / ISO 9001:2015

The Quality Management System Applies in the following area:

MAKRITE INDUSTRIES INC: Sales of Personal Protective Equipment(Fiber Mask, Filtering Respirator and Half Face Respirator)
and Houseware Products(Table Clothes, Placemat, Outdoor Cover, Shower Curtain and Other Related Products).
DONGGUAN SURE_ON PLASTIC & FIBER PRODUCTS CO., LTD: Design and Manufacture of the Exported Personal Protective
Equipment (Fiber Mask, Filtering Respirator and Half Face Respirator).
DONGGUAN MAKRITE INDUSTRIES CO.LTD.: Design and Manufacture Within The Scope of Qualification of Personal Protective
Equipment(Fiber Mask, Filtering Respirator and Half Face Respirator). Manufacture of Houseware Products(Table Clothes, Placemat,
Outdoor Cover, Shower Curtain and Other Related Products).

Certified since: December 30, 2013 Valid from: December 9, 2019 Valid until: December 29, 2022

After a surveillance cycle, the certificate is valid only when used together with an Acceptance Notice of Surveillance Audit issued by CQC.
Please access www.cqc.com.cn for checking validity of the certificate.

This certificate and its relevant information can query in the website of Certification and Accreditation Administration of the People's
Republic of China (www.cnca.gov.cn).



中国认可
国际互认
管理体系
MANAGEMENT SYSTEM
CNAS C001-M

陆梅
Signed by: Lu Mei



CHINA QUALITY CERTIFICATION CENTRE

Section 9, No.188, Nansihuan(the South Fourth Ring Road) Xilu(West Road), Beijing 100070,China

<http://www.cqc.com.cn>

A 0049753

2018年版



副本

QUALITY MANAGEMENT SYSTEM CERTIFICATE

Certificate No. 00119Q310176R2M/4400

We hereby certify that

**MAKRITE INDUSTRIES INC./DONGGUAN SURE_ON PLASTIC &
FIBER PRODUCTS CO.,LTD./DONGGUAN MAKRITE
INDUSTRIES LTD.**

Unified Social Credit Code: 9144190056665074X0

11F-5, No.79, Sec 1, Xin Tai 5th Road, XiZhi Dist., New Taipei City, Taiwan,R.O.C./ ZhuFo Ling Industrial Area,TangXia Town,DongGuan City,GuangDong,China / No.12, GuangYuan Street,168 Industrial Area, ZhuFo Ling,TangXia Town,DongGuan City,GuanDong,China

by reason of its
Quality Management System

has been awarded this certificate for compliance with the standard

GB/T 19001-2016 / ISO 9001:2015

The Quality Management System Applies in the following area:

MAKRITE INDUSTRIES INC: Sales of Personal Protective Equipment(Fiber Mask, Filtering Respirator and Half Face Respirator) and Houseware Products(Table Clothes, Placemat, Outdoor Cover, Shower Curtain and Other Related Products).
DONGGUAN SURE_ON PLASTIC & FIBER PRODUCTS CO., LTD: Design and Manufacture of the Exported Personal Protective Equipment (Fiber Mask, Filtering Respirator and Half Face Respirator).
DONGGUAN MAKRITE INDUSTRIES CO.LTD.: Design and Manufacture Within The Scope of Qualification of Personal Protective Equipment(Fiber Mask, Filtering Respirator and Half Face Respirator). Manufacture of Houseware Products(Table Clothes, Placemat, Outdoor Cover, Shower Curtain and Other Related Products).

Certified since: December 30, 2013 Valid from: December 9, 2019 Valid until: December 29, 2022

After a surveillance cycle, the certificate is valid only when used together with an Acceptance Notice of Surveillance Audit issued by CQC.

Please access www.cqc.com.cn for checking validity of the certificate.

This certificate and its relevant information can query in the website of Certification and Accreditation Administration of the People's Republic of China (www.cnca.gov.cn).



中国认可
国际互认
管理体系
MANAGEMENT SYSTEM
CNAS C001-M

陆梅
Signed by: Lu Mei



CHINA QUALITY CERTIFICATION CENTRE

Section 9, No.188, Nansihuan(the South Fourth Ring Road) Xilu(West Road), Beijing 100070,China

<http://www.cqc.com.cn>

A 0049752

2018年版



副本

质量管理体系认证证书

证书编号: 00119Q310176R2M/4400

兹证明

知勉工业股份有限公司/东莞迅安塑胶纤维制品有限公司/东莞知驿实业有限公司

统一社会信用代码: 9144190056665074X0

台湾新北市汐止区新台五路一段七十九号十一楼之五/中国广东省东莞市塘厦镇诸佛岭工业区/中国广东省东莞市塘厦镇诸佛岭 168 工业区广源街 12 号

建立的质量管理体系符合标准:

GB/T 19001-2016 / ISO 9001:2015

通过认证范围如下:

知勉工业股份有限公司: 劳保用品(纤维口罩、防护过滤口罩及半面罩)、家居用品(桌布、餐垫、户外套及浴帘等相关产品)的销售。

东莞迅安塑胶纤维制品有限公司: 出口劳保用品(纤维口罩、防护过滤口罩及半面罩)的设计和生

产。东莞知驿实业有限公司: 资质范围内劳保用品(纤维口罩、防护过滤口罩及半面罩)的设计和生, 家居用品(桌布、餐垫、户外套及浴帘相关产品)的生产。

首次发证日期: 2013年12月30日 本次发证日期: 2019年12月9日 有效期至: 2022年12月29日

在一个监督周期后, 本证书必须与CQC签发的监督审核合格通知书合并使用方可有效。查询证书有效状态请登陆www.cqc.com.cn。
本证书信息可在国家认证认可监督管理委员会官方网站 (www.cnca.gov.cn) 上查询



中国认可
国际互认
管理体系
MANAGEMENT SYSTEM
CNAS C001-M

陆梅
Signed by: Lu Mei



中国质量认证中心

中国·北京·南四环西路188号9区 100070
<http://www.cqc.com.cn>

A 0049752

2018年版



THE INTERNATIONAL CERTIFICATION NETWORK

CERTIFICATE

CQC has issued an IQNet recognized certificate that the organization:

MAKRITE INDUSTRIES INC./DONGGUAN SURE_ON PLASTIC & FIBER PRODUCTS CO.,LTD./DONGGUAN MAKRITE INDUSTRIES LTD.

11F-5, No.79, Sec 1, Xin Tai 5th Road, XiZhi Dist., New Taipei City, Taiwan, R.O.C./ ZhuFo Ling Industrial Area, TangXia Town, DongGuan City, GuangDong, China / No.12, GuangYuan Street, 168 Industrial Area, ZhuFo Ling, TangXia Town, DongGuan City, GuanDong, China

has implemented and maintains a

Quality Management System

for the following scope:

MAKRITE INDUSTRIES INC: Sales of Personal Protective Equipment(Fiber Mask, Filtering Respirator and Half Face Respirator) and Houseware Products(Table Clothes, Placemat, Outdoor Cover, Shower Curtain and Other Related Products).

DONGGUAN SURE_ON PLASTIC & FIBER PRODUCTS CO., LTD: Design and Manufacture of the Exported Personal Protective Equipment (Fiber Mask, Filtering Respirator and Half Face Respirator).

DONGGUAN MAKRITE INDUSTRIES CO.LTD.: Design and Manufacture Within The Scope of Qualification of Personal Protective Equipment(Fiber Mask, Filtering Respirator and Half Face Respirator). Manufacture of Houseware Products(Table Clothes, Placemat, Outdoor Cover, Shower Curtain and Other Related Products).

which fulfils the requirements of the following standard:

GB/T 19001-2016 / ISO 9001:2015

Issued on: December 9, 2019

Expires on: December 29, 2022

Registration Number: CN00119Q310176R2M/4400

This attestation is directly linked to the IQNet Partner's original certificate and shall not be used as a stand-alone document



Alex Stoichituiu
President of IQNet

Lu Mei
President of CQC



IQNet Partners*:

AENOR Spain AFNOR Certification France APCER Portugal CCC Cyprus CISQ Italy
CQC China CQM China CQS Czech Republic Cro Cert Croatia DQS Holding GmbH Germany FCAV Brazil
FONDONORMA Venezuela ICONTEC Colombia Inspecta Sertifiointi Oy Finland INTECO Costa Rica
IRAM Argentina JQA Japan KFQ Korea MIRTEC Greece MSZT Hungary Nemko AS Norway NSAI Ireland

NYCE-SIGE México PCBC Poland Quality Austria Austria RR Russia SII Israel SIQ Slovenia
SIRIM QAS International Malaysia SQS Switzerland SRAC Romania TEST St Petersburg Russia TSE Turkey YUQS Serbia
IQNet is represented in the USA by: AFNOR Certification, CISQ, DQS Holding GmbH and NSAI Inc.

* The list of IQNet partners is valid at the time of issue of this certificate. Updated information is available under www.iqnet-certification.com